

(Test of Q-bit Corporation report)

The transition verification test of the blood by “Q-Bit Air Cleaning & Aroma Emitting Device”

Purpose

After use front and use of light-quantum energy (Q-Bit Air Cleaning & Aroma Emitting Device), the state of the red corpuscles in blood is observed under a microscope, and change is checked.

unit used

Visual phase-contrast microscope x3600 time

Test method


One drop of blood is extracted from a left-hand middle finger leading-end part, and under a microscope, it expands by 3600 times and observes.

The status of the erythrocytes in blood is observed and compared in the status before a “Q-Bit Air Cleaning & Aroma Emitting Device” using, and the status after a using. mouse is used behind both ears, applying it to it for 30 minutes.



mouse busy condition

Test result

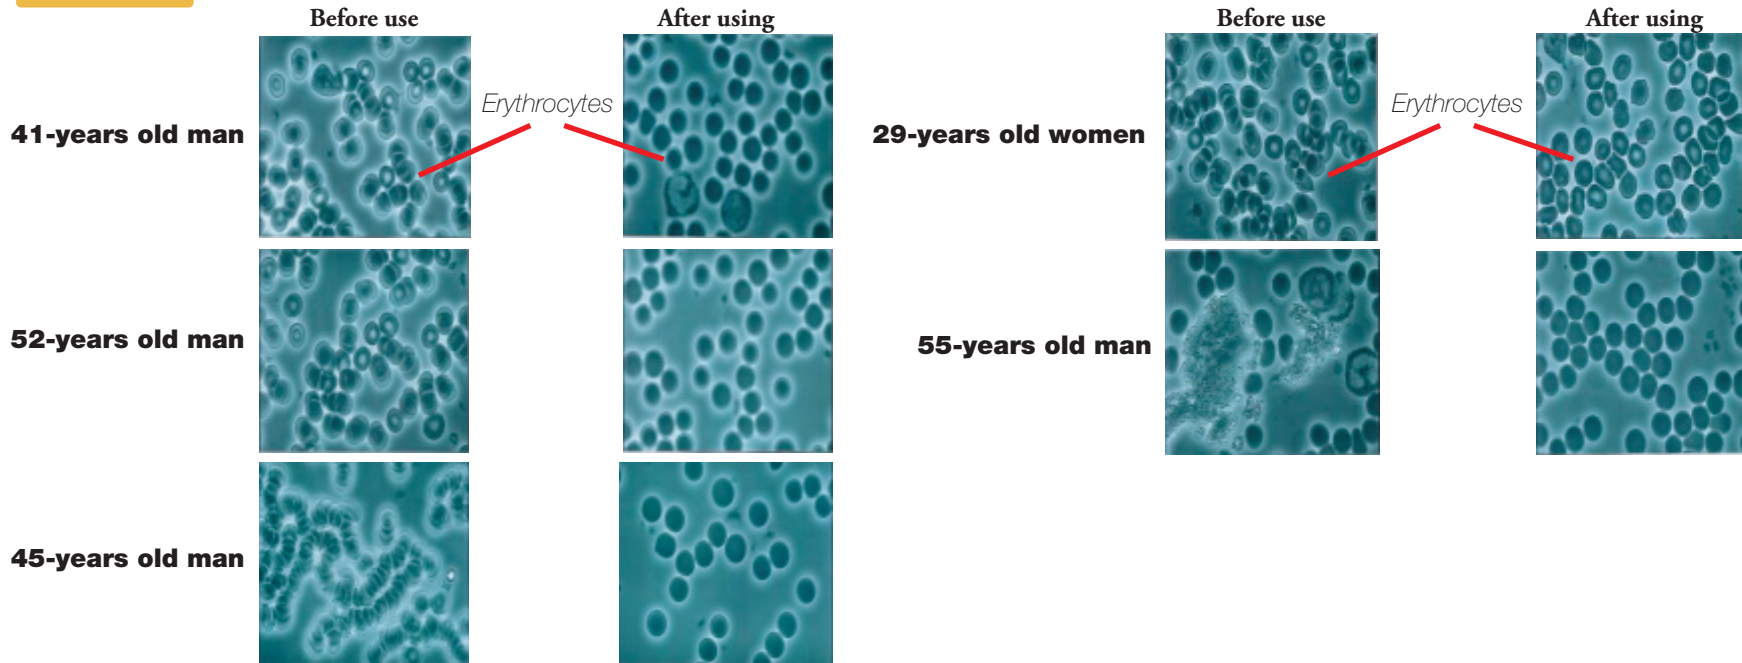

The blood chain decreased and it changed to blood with a deep color which is elastic round.